
Name:	**MIRANDA CARDENAS, LANDY RUBY**		**OD**	**OS**	
ID:	2046	Exam Date:	11/11/2025	11/11/2025	CZMI
DOB:	5/2/1962	Exam Time:	6:35 PM	6:45 PM	
Gender:	Female	Serial Number:	6000-11938	6000-11938	
Technician:	Operator, Cirrus	Signal Strength:	8/10	8/10	


ONH and RNFL OU Analysis:Optic Disc Cube 200x200 OD ● | ● OS

RNFL Thickness Map

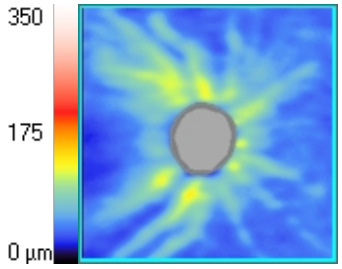


	OD	OS
Average RNFL Thickness	71 µm	86 µm
RNFL Symmetry	74%	
Rim Area	0.64 mm²	0.83 mm²
Disc Area	2.11 mm²	2.04 mm²
Average C/D Ratio	0.85	0.77
Vertical C/D Ratio	0.86	0.75
Cup Volume	0.863 mm³	0.604 mm³

RNFL Thickness Map

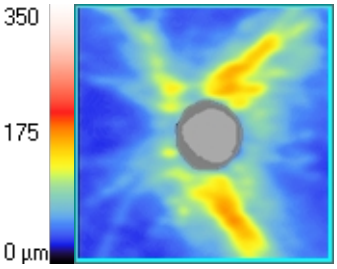


RNFL Deviation Map

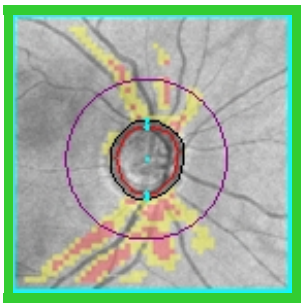


Disc Center(-0.15,-0.09)mm


Extracted Horizontal Tomogram

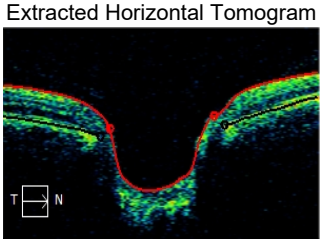


Extracted Vertical Tomogram

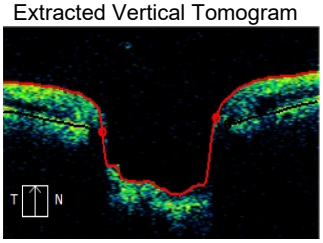


RNFL Circular Tomogram

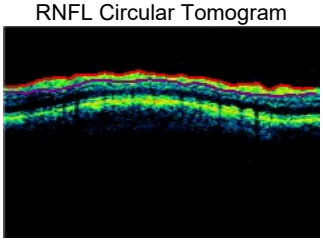


Neuro-retinal Rim Thickness

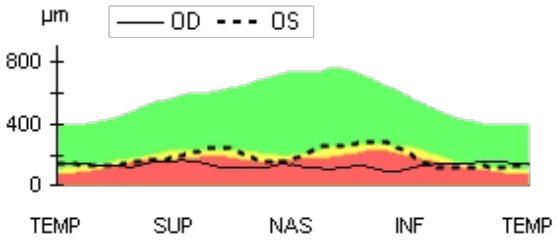


RNFL Thickness

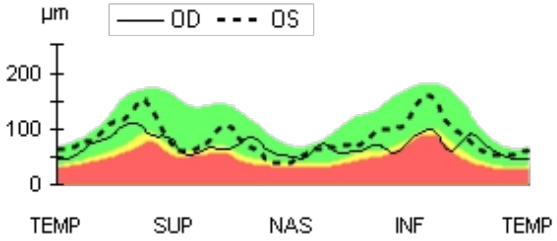

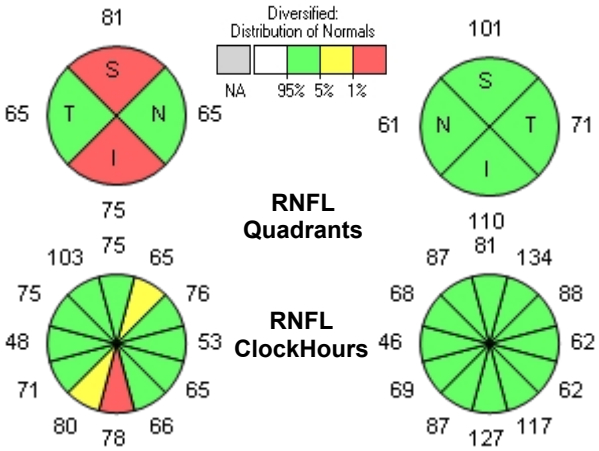


RNFL Deviation Map

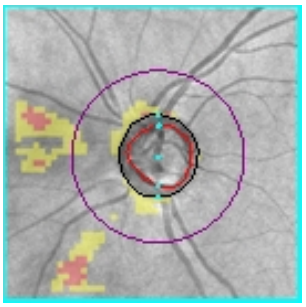


Disc Center(0.09,-0.03)mm


Extracted Horizontal Tomogram

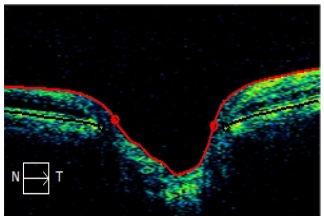

Extracted Vertical Tomogram

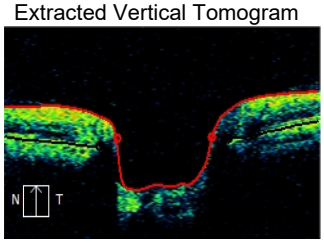

RNFL Circular Tomogram

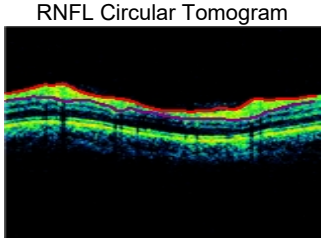

Comments

Doctor's Signature

SW Ver: 11.5.2.54532
Copyright 2020
Carl Zeiss Meditec, Inc
All Rights Reserved