
Name:	**BASTO BASTO, ANA MARIA**		**OD**	**OS**	
ID:	11862	Exam Date:	12/6/2025	12/6/2025	CZMI
DOB:	2/9/1939	Exam Time:	10:55 AM	10:58 AM	
Gender:	Female	Serial Number:	6000-11938	6000-11938	
Technician:	Operator, Cirrus	Signal Strength:	8/10	7/10	


ONH and RNFL OU Analysis:Optic Disc Cube 200x200 OD OS

RNFL Thickness Map

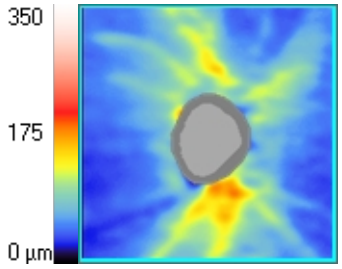


	OD	OS
Average RNFL Thickness	87 µm	75 µm
RNFL Symmetry	55%	
Rim Area	1.24 mm²	1.07 mm²
Disc Area	3.06 mm²	3.04 mm²
Average C/D Ratio	0.76	0.80
Vertical C/D Ratio	0.79	0.88
Cup Volume	0.409 mm³	0.456 mm³


RNFL Thickness Map

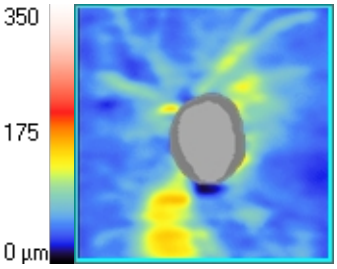


RNFL Deviation Map

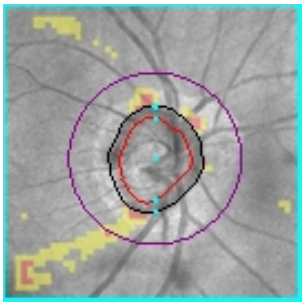

RNFL Deviation Map

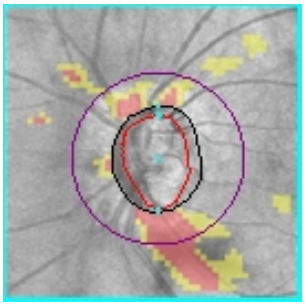


Neuro-retinal Rim Thickness

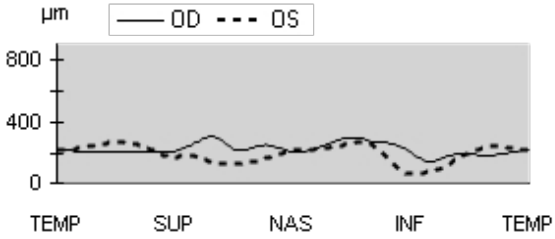


Disc Center(0.03,-0.09)mm

Extracted Horizontal Tomogram

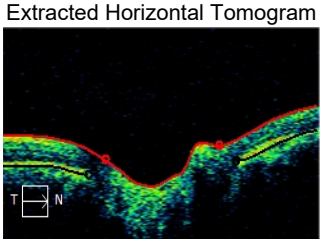


Disc Center(0.09,-0.09)mm


Extracted Horizontal Tomogram

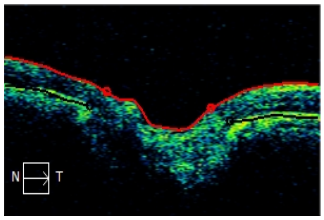


RNFL Thickness

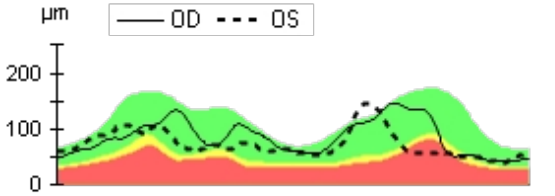


Extracted Vertical Tomogram

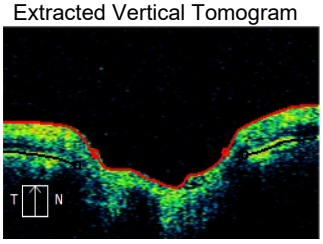


Extracted Vertical Tomogram

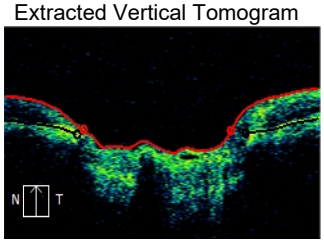

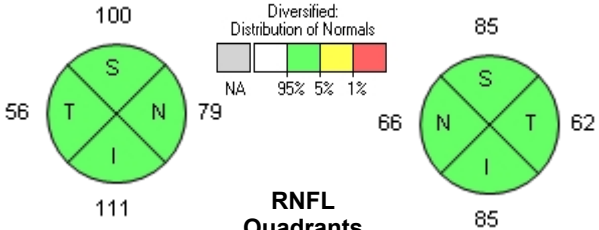


RNFL Quadrants


RNFL Circular Tomogram

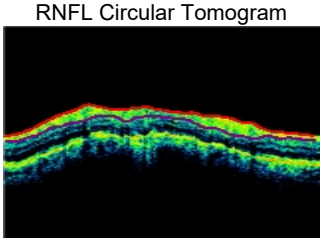

RNFL ClockHours

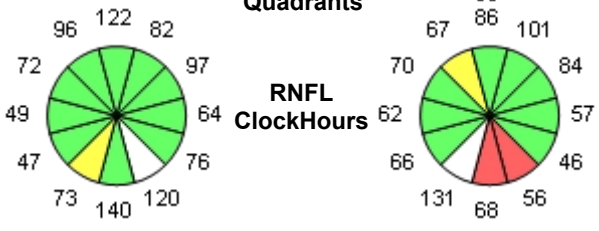

RNFL Circular Tomogram

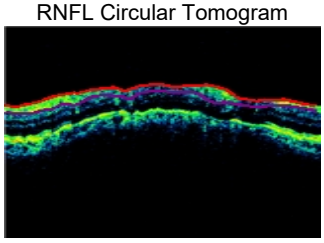

Comments

Doctor's Signature

SW Ver: 11.5.2.54532
Copyright 2020
Carl Zeiss Meditec, Inc
All Rights Reserved