
Name:	**DIAZ BARRAGAN, GABRIELLA ELIZETH**		**OD**	**OS**	
ID:	20065	Exam Date:	8/21/2026	8/21/2026	CZMI
DOB:	7/28/1979	Exam Time:	11:24 AM	11:29 AM	
Gender:	Female	Serial Number:	6000-11938	6000-11938	
Technician:	Operator, Cirrus	Signal Strength:	5/10	6/10	


ONH and RNFL OU Analysis:Optic Disc Cube 200x200 OD ● | ● OS

RNFL Thickness Map

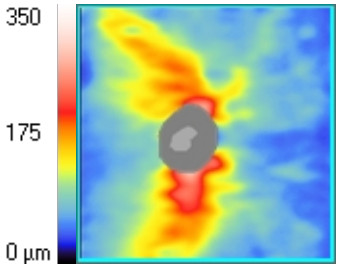


	OD	OS
Average RNFL Thickness	110 µm	100 µm
RNFL Symmetry	67%	
Rim Area	1.50 mm²	1.41 mm²
Disc Area	1.77 mm²	1.42 mm²
Average C/D Ratio	0.39	0.09
Vertical C/D Ratio	0.33	0.07
Cup Volume	0.057 mm³	0.000 mm³

RNFL Thickness Map

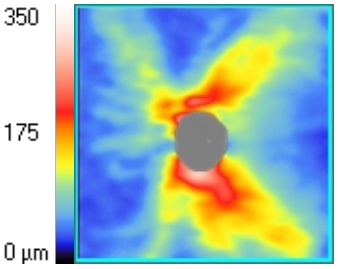


RNFL Deviation Map

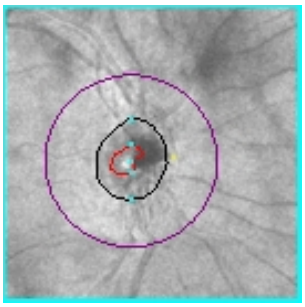


Disc Center(-0.45,-0.12)mm


Extracted Horizontal Tomogram

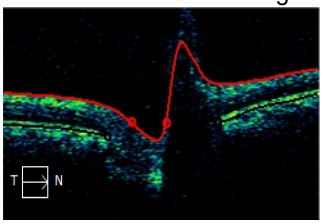


Extracted Vertical Tomogram

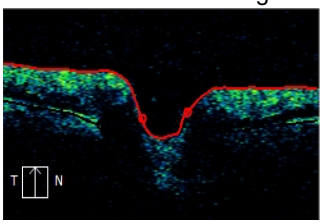


RNFL Circular Tomogram

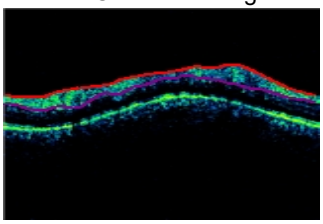


Neuro-retinal Rim Thickness

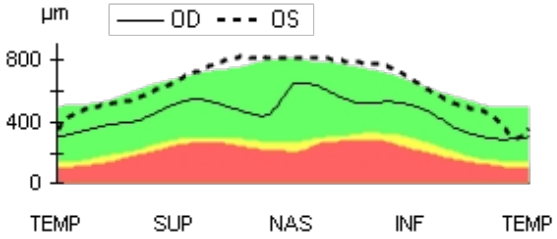


RNFL Thickness

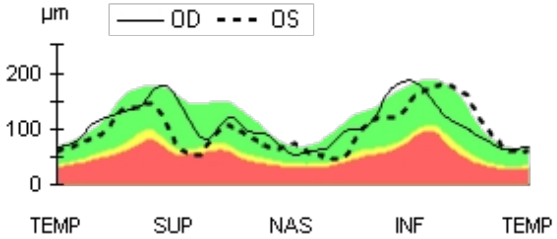

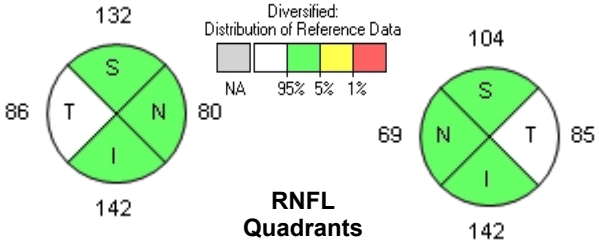


RNFL Quadrants

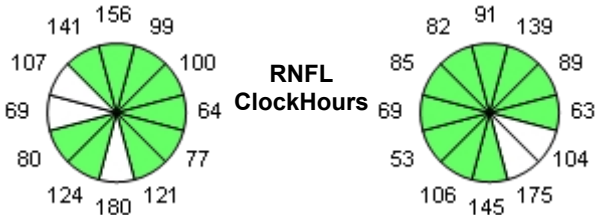


RNFL ClockHours

RNFL Deviation Map

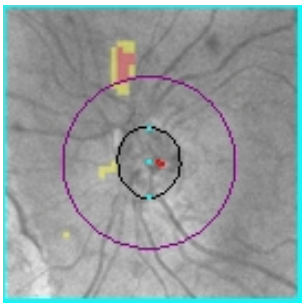


Disc Center(-0.09,-0.15)mm


Extracted Horizontal Tomogram

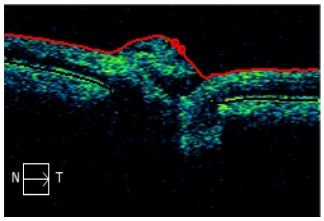

Extracted Vertical Tomogram

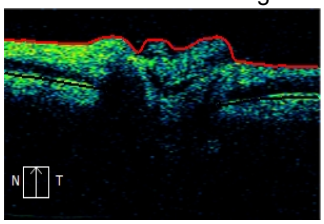

RNFL Circular Tomogram

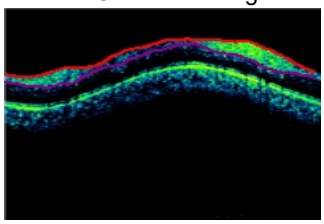

Comments

Doctor's Signature

SW Ver: 11.7.3.1019
Copyright 2025
Carl Zeiss Meditec, Inc
All Rights Reserved